	5 Committee Draft OIML/5CD  Date: 21 October, 2016 Reference number: TC_9_p1_N003  Supersedes document:
OIML TC 9 : Instruments for Measuring Mass and Density	Circulated to P- and O-members and liaison international bodies and external organizations for:  <div><input type="checkbox"/> P-members votes and comments</div> <div><input type="checkbox"/> O-members and liaisons comments</div> by: 27 January, 2017
Title: Metrological Regulation for Load Cells Part 3- Test report format  Clean version	
Convener: John Barton National Institute of Standards and Technology, USA	

TITLE OF THE CD (English): OIML R 60 <b>Metrological Regulation for Load Cells</b> <b>Part 3: Test report format</b>
TITRLE DU CD (French): OIML R 60 <b>Réglementation métrologique des cellules de pesée</b> <b>Partie 3: Format de Rapport pour l'examen de type</b>
Original version in: English

## Part 3 Test report format - General

### 1 Introduction

- 1.1 This Report Format applies to any kind of load cell (independent of its technology). It presents a standardized format for the results of the various tests and examinations, described in Part 2 of R 60, to which a type of load cell shall be submitted for the purpose of its approval based on this OIML Recommendation.
- 1.2 It is recommended that all metrology services or laboratories evaluating and/or testing types of load cells according to OIML R 60-1, or to national or regional regulations based on that Recommendation, use this Report Format, directly or after translation into a language other than English or French. In case of a translation, it is highly recommended to leave the structure and the numbers of the clauses unchanged: in this case, most of the content is also understandable for those who can not read the language of the translation.
- 1.3 Some of the tests may have to be repeated several times and reported using several identical sheets; therefore, report pages must be numbered in the space provided at the top of each page, completed by the indication of the total number of pages.
- 1.4 In the practical application of the Report Format, in addition to a cover page by the Issuing Authority, as a minimum, clauses A–F (as necessary) shall be included

#### 1. Applicability of this Report Format

In the framework of the *OIML Certificate System for Measuring Instruments*, and the *OIML Mutual Acceptance Arrangement (MAA)* applicable to load cells in conformity with OIML R 60 Parts 1 & 2, use of this report format is mandatory, in French and/or in English with translation into the national languages of the countries issuing such certificates, if appropriate.

Implementation of this Report Format is informative with regard to the implementation of OIML Recommendation R 60 parts 1 & 2 in national regulations.

##### 1.1. Calculation procedures

- 1.1.1. In order to facilitate a comparison of the reports established in English and in French, the same abbreviations (those of the English language) are used in both versions; the meanings of these abbreviations is given whenever appropriate.

In testing and evaluating load cells for pattern evaluation, it is recognized that the test apparatus and practices used by the various laboratories will be different. OIML R 60 allows for these variations and still provides a method for testing, recording and calculating results that are readily understandable by other knowledgeable parties reviewing the data.

In order to achieve this ease of comparability it is necessary that those persons conducting the tests use a common system for recording data and calculating results.

Thus, it is essential that the calculation procedures below be reviewed and followed closely in the completion of this test report.

### 1.1.2. Load cell errors ( $E_L$ = Error Load test)

- 1.1.2.1. Complete a Table 6.3 for each test temperature, calculate the averages and record in the right hand column. When five runs are necessary, use Table 6.4.
- 1.1.2.2. Determine the conversion factor,  $f$ , which is the number of indicated units per load cell verification interval,  $v$ , and is used to convert all “indicated units” to “ $v$ ”. It is determined from the test data averages of the increasing load tests at the initial 20 °C nominal test temperature.
- 1.1.2.3. If a test load corresponding to 75% of the measuring range for the load cell under test (i.e., 2 250 divisions for a 3 000 division cell, which is  $D_{\min}$  plus 75 % of the difference between  $D_{\max}$  and  $D_{\min}$ ) is not included in the test loads used in Table 4.10.1, interpolate between the adjacent upper and lower values of the averages of all three test runs and record in Table 4.10.3 (see R60-1: 8.8.2).
- 1.1.2.4. Calculate the difference between the average indication on the increasing load test runs at 75 % of the difference between  $D_{\max}$  and  $D_{\min}$  and the indication at  $D_{\min}$ . Divide the result (to five significant figures) by the number of verification intervals (75% of  $n$ ) for that load to obtain the conversion factor,  $f$ , and record in the tables that follow.

$$f = \frac{\text{average indication at } [D_{\min} + 0.75 \cdot (D_{\max} - D_{\min})]}{0.75 \cdot n}$$

The units of conversion factor  $f$  are indicated units (e.g. digits or counts) per load cell verification interval  $v$ .

- 1.1.2.5. Enter the average test indications of the tests at the temperatures following the initial test at a nominal 20 °C in Table 6.5. In recording this data, indicate a “no test load” indication (at  $D_{\min}$ ) as “0”. This may require subtracting the “no load indication at  $D_{\min}$ ” from the “test load indication” so that the first entry in the column is “0”. These “0’s” have been preprinted on the form to clarify that a dead load condition is recorded as “0”.
- 1.1.2.6. Calculate the reference indication,  $R_i$ , by converting the net test load, in mass units, to indicated units (e.g., counts or digits), by multiplying by the conversion factor,  $f$ , for each test load and recording in the 2nd column in Table 6.5.

$$R_i = \frac{(\text{test load } i - D_{\min})}{(D_{\max} - D_{\min})} \cdot n \cdot f$$

- 1.1.2.7. In Table 6.5 calculate the difference between the average test indication and the reference indication for each test load at each test temperature and divide the result by the conversion factor  $f$  to obtain the error,  $E_L$ , for each test load in terms of  $v$ .

$$E_L = (\text{average test indication for test load } i - \text{reference indication } R_i) / f$$

- 1.1.2.8. Compare  $E_L$  with the corresponding MPE for each test load.

**1.1.3. Repeatability error ( $E_R$  in terms of verification interval  $v$ )**

- 1.1.3.1. Enter data in Table 6.6.

- 1.1.3.2. Calculate the maximum difference between the indications of the on Form 6.3 and divide it by  $f$  to obtain the repeatability error,  $E_R$ , in terms of the load cell verification interval  $v$ .

$$E_R = (\text{maximum indication of the test load} - \text{minimum indication}) / f$$

- 1.1.3.3. Compare  $E_R$  with the absolute value of the corresponding MPE for each test load.

**1.1.4. Temperature effects on minimum dead load output (MDLO) ( $C_M$  = Change MDLO)**

- 1.1.4.1. Enter in Table 6.7 the average indication for the initial minimum test load,  $D_{\min}$ , for each test temperature from Table 6.3.

- 1.1.4.2. Calculate the difference between the average test indications for each temperature  $T_i$  in sequence and divide the result by the conversion factor  $f$  to obtain the change in terms of the load cell verification interval  $v$ .

$$C_M = (\text{average test indication at } T_2 - \text{average indication at } T_1) / f$$

- 1.1.4.3. Divide  $C_M$  by  $(T_2 - T_1)$  and multiply the result by 5 for class B, C, and D load cells or 2 for class A load cells. This gives the change in  $v$  per 5 °C for class B, C, and D load cells or in  $v$  per 2 °C for class A load cells.

- 1.1.4.4. Multiply the result by  $[(D_{\max} - D_{\min}) / n] / v_{\min}$  to give the final result  $C_M(v_{\min})$  in units of  $v_{\min}$  per 5°C for class B, C, and D load cells, or in units of  $V_{\min}$  per 2°C for class A load cells.  $C_M(v_{\min})$  must not exceed  $p_{LC}$ .

$$C_M(v_{\min}) = \frac{C_M \cdot (D_{\max} - D_{\min})}{n \cdot v_{\min}}$$

$$P_{LC} \leq C_M(v_{\min})$$

### 1.1.5. Creep magnitude $C_C(t)$ and minimum dead load output return ( $C_{DR}$ )

( $C_C(t)$  = Creep, expressed in terms of the load cell verification interval,  $v$ )

( $C_{DR}$  = DR, expressed in terms of the load cell verification interval,  $v$ )

Remark: Contrary to the minimum dead load output return DR in terms of mass the minimum dead load output  $C_{DR}$  is expressed in terms of the verification interval  $v$ ).

From the test indications recorded in Table 6.8, calculate the difference between the initial indication obtained at the minimum creep test load after the stabilization period and any indication obtained over the 30 minute test period with the maximum creep test load of 90% to 100% of  $E_{\max}$  and divide by the conversion factor the conversion factor  $f$ .

$$C_C = (\text{indication} - \text{initial indication}) / f$$

Remark: If the minimum creep test load or the maximum creep test load differ from  $D_{\min}$  or  $D_{\max}$  according to 2.1.2 "Load cell errors  $E_L$ " the conversion factor  $f$  must be recalculated with the minimum and maximum creep test loads (see 2.1.2.4).

1.1.5.1.  $C_C(t)$  must not exceed 0.7 times the absolute value of the MPE for the maximum creep test load at any time  $t$  over the 30 minute creep test period.

1.1.5.2. Calculate the difference between the test indications obtained at  $t = 20$  minutes and  $t = 30$  minutes after the initial indication at  $t = t_0$  and divide by  $f$  to obtain the creep error,  $C_C(30 - 20)$ , in terms of the load cell verification interval  $v$ .

$$C_C(30 - 20) = (\text{indication at time } t = 30 \text{ minutes} - \text{indication at time } t = 20 \text{ minutes}) / f$$

1.1.5.3.  $C_C(30 - 20)$  shall not exceed 0.15 times the absolute value of the MPE for the applied load.

1.1.5.4. Calculate the difference between the initial indication obtained at the minimum creep test load after the stabilization period ( $t_0 = 0$  min) and the indication at the minimum creep test load after the creep test and after a time interval for stabilization ( $t > 30$  min) and divide the result by conversion factor  $f$  to obtain the minimum dead load output return,  $C_{DR}$ , in terms of  $v$ .

$$C_{DR} = (\text{indication at the minimum creep test load indication} - \text{initial indication at the minimum creep test load indication}) / f$$

1.1.5.5. If the time intervals specified in R60-1: Table 7 have been met,  $C_{DR}$  must not exceed 0.5  $v$ .

1.1.5.6. If the actual time is between 100 % and 150 % of the specified time in R60-1: Table 7, then the following applies:

$$C_{DR} \leq 0.5 (1 - (x - 1))$$

with

$$x = \text{actual time / specified time}$$

- 1.1.5.7. Whereas  $C_{DR}$  expresses the minimum dead load output return in terms of  $v$ , the value of  $D_R$  as used in the OIML R76 is expressed in units of mass (g, kg or t).
- 1.1.5.8. Calculate the minimum dead load output return,  $DR$ , expressed in units of mass (g, kg or t) as follows:  $DR = (E_{\max} - C_{DR}) / n_{LC}$
- 1.1.5.9. Regardless of the value declared by the manufacturer for the apportionment factor,  $p_{LC}$ , the MPE for creep shall be determined from R60-1: Table 4 using the apportionment factor,  $p_{LC} = 0.7$  (see R60-1: 5.5.1).

#### 1.1.6. Barometric pressure effects<sup>1</sup> (CP = Change Due to Barometric Pressure)

- 1.1.6.1. From the test indications recorded in Table 6.9, calculate the difference between the indications for each pressure and divide the result by conversion factor  $f$  to obtain the change,  $CP$ , in terms of  $v$ .

$$C_P = (\text{indication at } P_2 - \text{indication at } P_1) / f$$

- 1.1.6.2. Divide  $C_P$  by  $(P_2 - P_1)$  to determine the change due to barometric pressure in terms in terms of  $v$  per kilopascal (kPa).
- 1.1.6.3. Multiply the result by  $[(E_{\max} - E_{\min}) / n_{LC}]$  to obtain the result in units of mass (g, kg, or t) per kPa (as stated by the manufacturer). The result must not exceed  $v_{\min}$ .

$$C_P(v_{\min}) = \frac{C_P}{(P_2 - P_1)} \cdot \frac{(E_{\max} - E_{\min})}{n_{\max}} \leq v_{\min}$$

#### 1.1.7. Humidity effects<sup>2</sup> (CH or no mark)

( $C_{H\min}$  = Change in terms of  $v$  due to Humidity effects on the indication of the minimum test load  $D_{\min}$ )

( $C_{H\max}$  = Change due to Humidity effect on the indication of the maximum test load  $D_{\max}$ )

Remark: If the minimum or maximum test load used for this test differ from the minimum test load  $D_{\min}$  or maximum test load  $D_{\max}$  according to 2.1.2 "Load cell errors  $E_L$ " the conversion factor  $f$  must be recalculated with the minimum and maximum test loads of this test (see 2.1.2.4).

<sup>1</sup> This test may not be necessary depending on the design of the load cell.

<sup>2</sup> This test is not necessary if the load cell is marked NH or SH.

- 1.1.7.1. From the test indications recorded in Table 6.10.1, calculate the difference between the initial indications for the minimum test load,  $D_{\min}$ , before and after the damp heat test and divide the result by conversion factor  $f$  to obtain the change,  $C_{H\min}$ , in terms of verification interval  $v$  (see R60-1: 5.6.3.1).

$C_{H\min}$  must not exceed  $0.04 \cdot n$ .

- 1.1.7.2. Calculate the average indications  $\bar{I}\{D_{\max}\}$  and  $\bar{I}\{D_{\min}\}$  at  $D_{\min}$  and  $D_{\max}$  (see R60-1: 8.10.5) for the required number of test indications, before and after the damp heat test. Subtract  $\bar{I}\{D_{\max}\}$  from  $\bar{I}\{D_{\min}\}$  for the tests before and after damp heat test and then calculate the difference between the results. Divide the result by the conversion factor  $f$  to obtain the change,  $C_{H\max}$ , in terms of  $v$ .

$$C_{H\max} = \frac{[(\bar{I}\{D_{\max}\} - \bar{I}\{D_{\min}\})_{\text{after}} - (\bar{I}\{D_{\max}\} - \bar{I}\{D_{\min}\})_{\text{before}}]}{f}$$

- 1.1.7.3.  $C_{H\max}$  must not exceed the MPE (see table 4 in 5.3.1.1).

### 1.1.8. Humidity effects<sup>3</sup> (SH)

Report load test errors at different temperatures and humidity conditions using Forms 6.3, then indicate the results in Table 6.10.2 utilizing the procedure contained within “load cell errors” procedure, 2.1.2, in a manner similar to that used for the preparation of Table 6.5.

## 1.2. Additional tests for digital load cells

### 1.2.1. Warm-up time

- 1.2.1.1. Enter data on Form 6.11.
- 1.2.1.2. Span is the result of subtraction of the indication at the minimum test load,  $D_{\min}$ , from the indication at the maximum test load,  $D_{\max}$ .
- 1.2.1.3. Change is the difference between the span and the initial run span.

### 1.2.2. Power voltage variations

- 1.2.2.1. Enter data on Form 6.12.
- 1.2.2.2. Perform load tests and record results utilizing Form 6.12.
- 1.2.2.3. Calculate reference indications in accordance with the “load cell errors” procedure, 2.1.2.
- 1.2.2.4. Indicate results on Form 6.12.

### 1.2.3. Short-time power reductions

---

<sup>3</sup> This test is not necessary if the load cell is marked NH or CH or has no humidity marking.

1.2.3.1. Enter data on Form 6.13.

1.2.3.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$

1.2.3.3. Indicate results on Form 6.13.

#### 1.2.4. Bursts (electrical fast transients)

1.2.4.1. Enter data on Forms 6.14.1 and 6.14.2.

1.2.4.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$

1.2.4.3. Indicate results on Forms 6.14.1 and 6.14.2.

#### 1.2.5. Surge

1.2.5.1. Enter data on Forms 6.15

1.2.5.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$

1.2.5.3. Indicate results on Forms 6.15

#### 1.2.6. Electrostatic discharge

1.2.6.1. Enter data on Forms 6.16.1, 6.16.2 and 6.16.3.

1.2.6.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$

1.2.6.3. Indicate results on Forms 6.16.1, 6.16.2.1, and 6.16.2.2.

1.2.6.4. Provide test point information on Form 6.16.3.

#### 1.2.7. Electromagnetic susceptibility

1.2.7.1. Enter data on Form 4.10.15(a).

1.2.7.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$



1.2.7.3. Indicate results on Form 6.17.1.

1.2.7.4. Provide test set-up information on Form 6.17.2.

**1.2.8. Immunity to conducted electromagnetic fields**

1.2.8.1. Enter data on Form 6.18.

1.2.8.2. Calculate the difference, which is:

$$\text{difference} = \frac{(\text{indication with disturbance, in units} - \text{indication without disturbance, in units})}{\text{conversion factor, } f}$$

1.2.8.3. Indicate results on Form 6.18.

1.2.8.4. Provide test set-up information on Form 6.18.

**1.2.9. Span stability**

1.2.9.1. Enter data on Forms 6.19.1 (3 runs) to 6.19.2 (5 runs).

1.2.9.2. Calculate averages and record on Forms 6.19.1 (3 runs) to 6.19.2 (5 runs).

1.2.9.3. Indicate results on Form 6.19.3

**1.3. General notes**

**1.3.1.** Absolute (not relative) time shall be recorded.

**1.3.2.** The testing laboratory may submit any graphs or plots depicting the test results on the following pages of this report.

Note: For example, Figure 1 gives a sample plot depicting the combined errors versus applied load.

**1.3.3.** When reporting values for individual test data, the data should be truncated to two significant digits to the right of the decimal place and reported in load cell verification intervals,  $v$ .

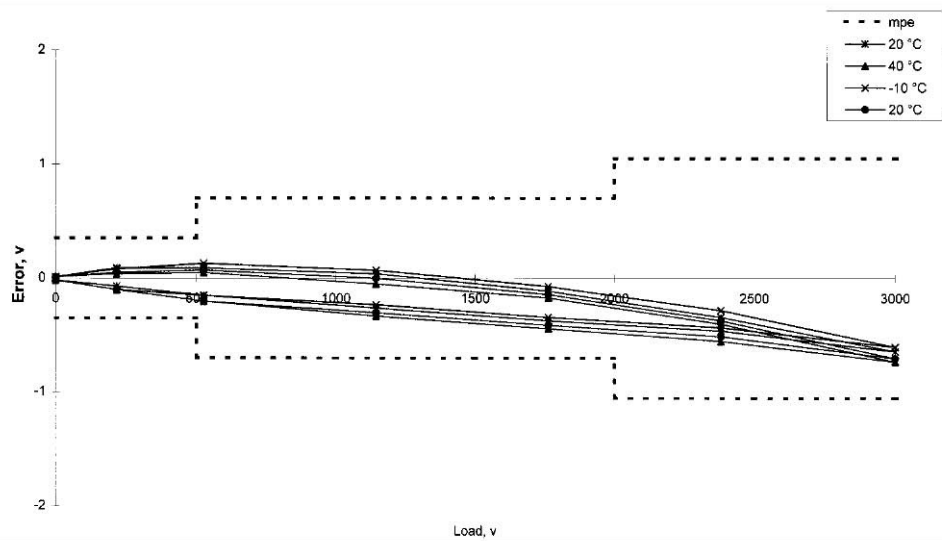


Figure 1 Example of an error envelope

## 1.4. Formula signs and list of symbols

<i>Symbol</i>	<i>Description</i>	<i>Reference</i>
$C_C(t)$	creep magnitude, expressed in terms of $v$ at time $t$ obtained over the 30 minutes creep test	2.1.5
$C_C(30 - 20)$	difference between output at $t = 30$ minutes and at $t = 20$ minutes during creep test	2.1.5.2
$C_{DR}$	minimum dead load output return, expressed in terms of $v$	2.1.5
$C_{Hmax}$	humidity effect on maximum test load output, expressed in terms of $v$	2.1.7
$C_{Hmin}$	humidity effect on minimum test load output, expressed in terms of $v$	2.1.7
$C_M$	temperature effect on minimum dead load output, expressed in terms of $v$	2.1.4
$C_M(v_{min})$	temperature effect on minimum dead load output, expressed in terms of $v_{min}$ per 5°C for class B, C and D or per 2°C for class A.	2.1.4
$C_P$	barometric pressure effect, expressed in terms of $v$	2.1.6
$C_P(v_{min})$	barometric pressure effect, expressed in terms of mass (g, kg, t) per kPa.	2.1.6
$D_{max}$	maximum test load	R60-1, 3.5.6
$D_{min}$	minimum test load	R60-1, 3.5.12
$DR$	minimum dead load output return, expressed in mass units (g, kg, t)	R60-1, 3.5.10
$E_L$	load cell error, expressed in terms of $v$	2.1.2
$E_{max}$	maximum capacity of the load cell	R60-1, 3.5.5
$E_{min}$	minimum dead load of the load cell	R60-1, 3.5.9
$E_R$	repeatability error, expressed in terms of $v$	2.1.3
$f$	conversion factor, number of indicated units per verification interval, $v$	2.1.2.4
$mpe$	maximum permissible error	R60-1, 3.7.10
$n$	number of load cell verification intervals into which the load cell measuring range is divided	R60-1 3.5.13
$n_{LC}$	maximum number of load cell verification intervals	R60-1, 3.5.8
$p_{LC}$	apportionment factor	R60-1, 3.7.2
$R_i$	reference indication (net test load), expressed in indication units	2.1.2.6
$t_0$	Time $t_0 = 0$ min when the initial indication at minimum test load is measured	2.1.5
$t$	Time over the 30 minute creep test period after the initial indication ( $t_0 = 0$ min) at minimum test load	2.1.5
$T_1, T_2$	temperature1, temperature2	2.1.4.2
$v$	load cell verification interval	R60-1, 3.5.4
$v_{min}$	minimum load cell verification interval	R60-1, 3.5.11
$Y$	relative $v_{min}$ , $Y = E_{max}/v_{min}$	R60-1, 3.5.15,
$Z$	relative DR, $Z = E_{max}/(2 \times DR)$	R60-1, 3.5.14

## 1.5. Summary of formulae contained within calculation procedures

<i>Symbol</i>	<i>Formula</i>
$C_C$	$C_C = (\text{indication} - \text{initial indication}) / f$
$C_C(30 - 20)$	$C_C(30 - 20) = (\text{test indication at 30 minutes} - \text{test indication at 20 minutes}) / f$
$C_{DR}$	$C_{DR} = (\text{minimum test load indication}_2 - \text{minimum test load indication}_1) / f$
$C_{Hmin}$	$C_{Hmin} = [(\text{indication at } D_{min})_{after} - (\text{indication at } D_{min})_{before}] / f$
$C_{Hmax}$	$C_{Hmax} = [(\text{indication at } D_{max} - \text{indication at } D_{min})_{after} - (\text{indication at } D_{max} - \text{indication } D_{min})_{before}] / f$
$C_M$	$C_M = (\text{indication at } T_2 - \text{indication at } T_1) / f$
$C_P$	$C_P = (\text{indication at } P_2 - \text{indication at } P_1) / f$
$DR$	$DR = E_{max} \times C_{DR} / n_{LC}$
$E_L$	$E_L = (\text{average test indication} - \text{reference indication}) / f$
$E_R$	$E_R = (\text{maximum indication} - \text{minimum indication}) / f$
$f$	$f = [\text{indication at 75 \% of } (D_{max} - D_{min}) - \text{indication at } D_{min}] / (0.75 \times n) \text{ [see Note 2]}$
$R_i$	$R_i = [(\text{test load} - D_{min}) / (D_{max} - D_{min})] \times n \times f$

*Notes:* 1 Observe extreme caution by referring to calculation procedure for correct application of these formulae.

2 Use with initial 20 °C ascending load run only. Refer to R60-1: 8.8.2.

## 2. Guidance for the application of this Test Report Format

In case a prescribed test is not relevant for the type of instrument to be tested, the reason why the test is omitted shall be clearly stated in the field “Remarks” (for instance surge tests on signal lines shorter than 30 m, tests related to AC mains supply in case of an instrument only powered by batteries, or partial testing after modification of a previously tested type).

The number of the report and the page numbers shall be completed in the heading.

Page 1 of this Report Format may be replaced by a cover page by the Issuing authority.

Enter “NA” or “/” for “the test is not applicable.”

### **3. The Evaluation Report**

**Cover page**  
**by the**  
**Issuing Authority**

**3.1. Authority, responsible for this Report:**

Name	
Address	
Report number	
Application number	
Period of tests	
Date of issuing this Report	
Name and signature of the responsible person	
Stamp(s) (if applicable)	

**3.2. Synopsis of the results of the examination and tests**

The load cell under test fulfills <b><u>ALL</u></b> the applicable requirements according to OIML R60 (201X):	Yes <input type="checkbox"/>	No <input type="checkbox"/>
Remarks:		

### 3.3. Summary of the results of the examination and tests

*(To be completed by the Issuing Authority)*

#### 3.3.1. Examinations

For details, refer to the tests as indicated in the last column.

<i>General requirements:</i>	Passed	Failed	Details in R60Parts1&2
Documentation			8.5
Inscription and presentation of load cell information			6.2

#### 3.3.2. Performance tests *(Refer to 9.7 of OIML R60-1)*

For details, refer to the tests as indicated in the last column.

Tests performed at (20°C / X<sub>1</sub>°C / X<sub>2</sub>°C / 20°C):

Test procedure	Passed	Failed	Details in R60-Parts1&2
Maximum permissible measurement errors			5.3 / 8.10.1
Repeatability error			5.4 / 8.10.1
Temperature effect on minimum dead load output return			5.6.1.3 / 8.10.1
Creep test			5.5.1 / 8.10.2
Minimum dead load output return (DR)			5.5.2 / 8.10.3
Barometric pressure effects at ambient temperature			5.6.2 / 8.10.4
Humidity effects (CH, SH)			5.6.3 / 8.10.5 / 8.10.6

*Additional tests performed for digital load cells:*

Test procedure	Passed	Failed	Details in R60-Parts1&2
Warm-up time			5.7.2.1 / 8.10.7.3
Power Voltage Variations			5.7.2.2 / 5.7.2.3 / 5.7.2.4 / 8.10.7.4
Short-time power reductions			5.7.2.5 / 8.10.7.5
Bursts (electronical fast transients)			5.7.2.5 / 8.10.7.6
Surge			5.7.2.5 / 8.10.7.7
Electrostatic discharge			5.7.2.5 / 8.10.7.8
Electromagnetic susceptibility			5.7.2.5 / 8.10.7.9
Immunity to conducted electromagnetic fields			5.7.2.5 / 8.10.7.10
Span stability			6.7.2.6 / 8.10.7.11
Software			6.1

**3.4. General Information regarding the evaluation process****3.4.1.** *Manufacturer of the specimen*

Company	
Address	
Contact Information	



**3.4.2. Applicant**

Company		
Representative (name, telephone)		
Address		
Contact Information		
Reference		
Date of application		
Application number		
Applicant authorized by the manufacturer (documented)	<input type="checkbox"/> Yes <input type="checkbox"/> No	
Statement that no concurrent application for OIML type evaluation has been made to any other OIML Issuing Authority (see OIML B3, 5.1.2 b)	<input type="checkbox"/> Yes <input type="checkbox"/> No	
Remarks:		

### 3.4.3. Testing laboratories involved in the tests

(This table has to be completed for each test laboratory)

Name			
Address			
Application number			
Tests by this laboratory			
Date/period of tests			
Name(s) of test engineer(s)			
Accredited by		Number:	Expires (date):
Accreditation includes R60	<input type="checkbox"/> Yes      Edition: <input type="text"/> <input type="checkbox"/> No		
Details of relevant peer assessment or assessment by other means			
In case tests have been performed at locations other than the address of this laboratory, give details here			
Name of the responsible person			
Date of signature			
Stamp (if applicable) and signature of the responsible person			
<i>Remarks:</i>			

**3.5. General information concerning the load cell type***(as provided by the manufacturer prior to the evaluation)*

Manufacturer's name/trade mark	
Manufacturer's type designation (or load cell model number)	

	Unit	Range
Accuracy classes		
Maximum number of verification intervals $n_{LC}$		
Maximum capacity $E_{max}$	(g, kg, t)	
Minimum capacity $E_{min}$	(g, kg, t)	
Minimum load cell verification interval $v_{min}=(E_{max} / Y)$	(g, kg, t)	
Minimum dead load output return $DR = (1/2 \cdot E_{max} / Z)$	(g, kg, t)	
Rated output	(mV/V or counts)	
Input Impedance	$\Omega$	

**3.6. Accessories, supplied with the test pattern by the applicant**

Accessory	Remarks and specifications
Analog data processing device ( <i>see OIML R76, T.2.2.3</i> )	
Cables	
Load cell mounting hardware:	
Load introduction elements:	
Main power supply	
Battery (type, voltage)	
Indicator ( <i>see OIML R76, T.2.2.2</i> )	
Data printer	
Other accessories:	

Further remarks concerning accessories:

---



---



---



---



---



---



---

**3.7. Selection of sample(s) tested****3.7.1.** Definition of the test pattern (*supplied by the applicant for this test report*)

This test report is issued for the following load cell:

Model designation	Serial number	Maximum capacity	Maximum number of load cell intervals	Minimum load cell verification interval	Minimum dead load output return
		$E_{\max}$ (g, kg or t)	$n_{LC}$	$V_{\min}$ (g, kg or t)	DR (g, kg or t)

**3.7.2.** Justification of the selection of the test sample(s)  
(*refer to R60-2: 8.3, 8.4 and Annex D*):

Model designation	Serial number	Justification / Remark	Test Report No. (if available)

**3.8. Adjustments and modifications made to the samples during the testing:**

*Justification of the selection of the test sample(s) (refer to R60 part 2: 8.3):*

Model designation	Serial number	Adjustments and modifications made to the samples	Test Report No. (if available)

*Further information concerning adjustments:*

---

---

---

---

---

---

---

---

---

---

### 3.9. Additional information concerning the type

#### 3.9.1. General information of the load cell under test (specified by the manufacturer)

Manufacturer's name/trade mark		
Manufacturer's type designation (or load cell model number)		
Serial number		
Load cell construction ( <i>e.g. S-type, ring type, bending beam</i> )		
Load cell material		
Sealing of strain gauge application ( <i>e.g. hermetically, potted</i> )		
Digital load cell ( <i>Yes / no</i> )		
Accuracy classes		
Maximum number of verification intervals $n_{LC}$		
Maximum capacity $E_{max}$	(g, kg, t)	
Minimum capacity $E_{min}$	(g, kg, t)	
Minimum load cell verification interval $v_{min} = (E_{max} / Y)$	(g, kg, t)	
Minimum dead load output return $DR = (1/2 \cdot E_{max} / Z)$	(g, kg, t)	
Rated output	(mV/V or counts)	
Input Impedance <sup>1</sup>	$\Omega$	
Cable connection <sup>1</sup>		4-wire / 6-wire
Cable length <sup>2</sup>	m	

<sup>1</sup> mandatory for strain gauge load cells

<sup>2</sup> mandatory for strain gauge load cells with 4-wire connection

Additional information concerning the type (connection equipment, interfaces, etc.):

---

---

---

---

---

---

---

---

### 3.9.2. Additional information for the performance tests

(ref. R60 part 1, clauses 6.2.2, 6.2.3, and 6.2.4)

Accuracy class	<input type="checkbox"/> A	<input type="checkbox"/> B	<input type="checkbox"/> C	<input type="checkbox"/> D
Working temperature (if other than $-10^{\circ}\text{C}$ to $+40^{\circ}\text{C}$ ): Upper _____ $^{\circ}\text{C}$ , Lower _____ $^{\circ}\text{C}$				
Humidity symbol	<input type="checkbox"/> NH	<input type="checkbox"/> SH	<input type="checkbox"/> CH or no marking	
Loading designation: (ref. R60 part 1 clause 6.2.4.2)				
Tension <input type="checkbox"/> Compression <input type="checkbox"/> Universal <input type="checkbox"/> Beam (shear) <input type="checkbox"/> Beam (bending) <input type="checkbox"/>				
Minimum dead load as: $E_{\min} =$				
Safe load limit as: $E_{\lim} =$				
Excitation Voltage: <input type="checkbox"/> AC <input type="checkbox"/> DC				
Value of the apportionment factor, $p_{\text{LC}}$ , if not equal to 0.7				





**3.9.6.** Inscriptions and presentations of load cell information  
(according to manufacturer statement, see OIML R60 part 1, 6.2)

<b>R60 part 1 reference</b>	<b>Information</b>	<b>On the load cell</b>	<b>Accompanying document</b>	<b>In the Data sheet</b>
6.2.1 / 6.2.2	Name or trademark of manufacturer			
6.2.1 / 6.2.2	Manufacturer's own designation or load cell model			
6.2.1	Serial number			<i>Not applicable</i>
6.2.1	Year of production			<i>Not applicable</i>
6.2.1	OIML certificate number			
6.2.2 / 6.2.4.1	Accuracy class(es) and their symbols			
6.2.4.5	Maximum number of load cell verification intervals, $n_{LC}$			
6.2.2 / 6.2.4.2	Type of load			
6.2.2 / 6.2.4.3	Working temperature designation			
6.2.2 / 6.2.4.4	Humidity symbol "NH"			
6.2.2 / 6.2.4.4	Humidity symbol "SH"			
6.2.2 / 6.2.4.4	No humidity symbol or "CH"			
6.2.2	Minimum dead load, $E_{min}^{1)}$			
6.2.1 / 6.2.2	Maximum capacity, $E_{max}^{1)}$			
6.2.2	Safe load limit, $E_{lim}^{1)}$			
6.2.2	Minimum load cell verification interval ( $v_{min}$ ) <sup>1)</sup>			
6.2.3, a	Relative $v_{min}$ (Y)			
6.2.3, b	Minimum dead load return DR <sup>1)</sup>			
6.2.3, b	Relative DR (Z)			
6.2.2, l	Rated output			
6.2.2, l	Excitation voltage			
6.2.2, l	Input impedance			
6.2.2, l	Cable connection <sup>2)</sup>			
6.2.2, l	Cable length <sup>3)</sup>			
6.2.2, k	Apportionment factor, $p_{LC}$ (if not equal to 0.7)			
6.2.2, l, 6.2.3, c	Further information			

<sup>1)</sup> In units of (g, kg, t)

<sup>2)</sup> E.g. 4-wire / 6-wire cable

<sup>3)</sup> mandatory for strain gauge load cells with 4-wire connection

*Further load cell information given by the manufacturer:*

---



---



---



---



---



---



---




---

**3.9.7.** Various designs within the model range:

Model designation	Maximum capacity	Minimum dead load	Maximum number of load cell intervals	Minimum load cell verification interval	Minimum dead load output return
	$E_{\max}$ (g, kg or t)	$E_{\min}$ (g, kg or t)	$n_{LC}$	$v_{\min}$ (g, kg or t)	DR (g, kg or t)

**3.9.8.** Relevant photographs / documentation of the model range:



**3.9.9.** Definition of load cell families / construction

*(This table to be completed by the manufacturer for each load cell family within the model range)*

Type / Model designation	specification	OIML R60 part 1	Remark
	Application of load	3.2.1	<i>(e.g. tension / compression)</i>
	Load cell construction	3.3	<i>(e.g. bending beam)</i>
	Material or combination of materials	3.4.2	
	Shape	3.4.2	See 4.9.10
	Design of measuring technique	3.3.1	<i>(e.g. strain gauge bonded to metal)</i>
	Sealing of strain gauges	3.4.2	
	Mounting method	Annex E	
	Load transmission	Annex E	See 4.9.11
	Output rating	3.4.2	
	Supply voltage	3.4.2	
	Input impedance	3.4.2	
	Cable connection	3.4.2	
	Cable length <sup>1</sup>	3.4.2	

*Further remarks concerning the definition of load cell families / construction (see table above)*

---



---



---



---



---



---




---

<sup>1</sup> mandatory for strain gauge load cells with 4-wire connection

**3.9.10.** Load cell dimensions within the load cell family

*Pictures / Drawings of the load cell dimensions of the load cell family*

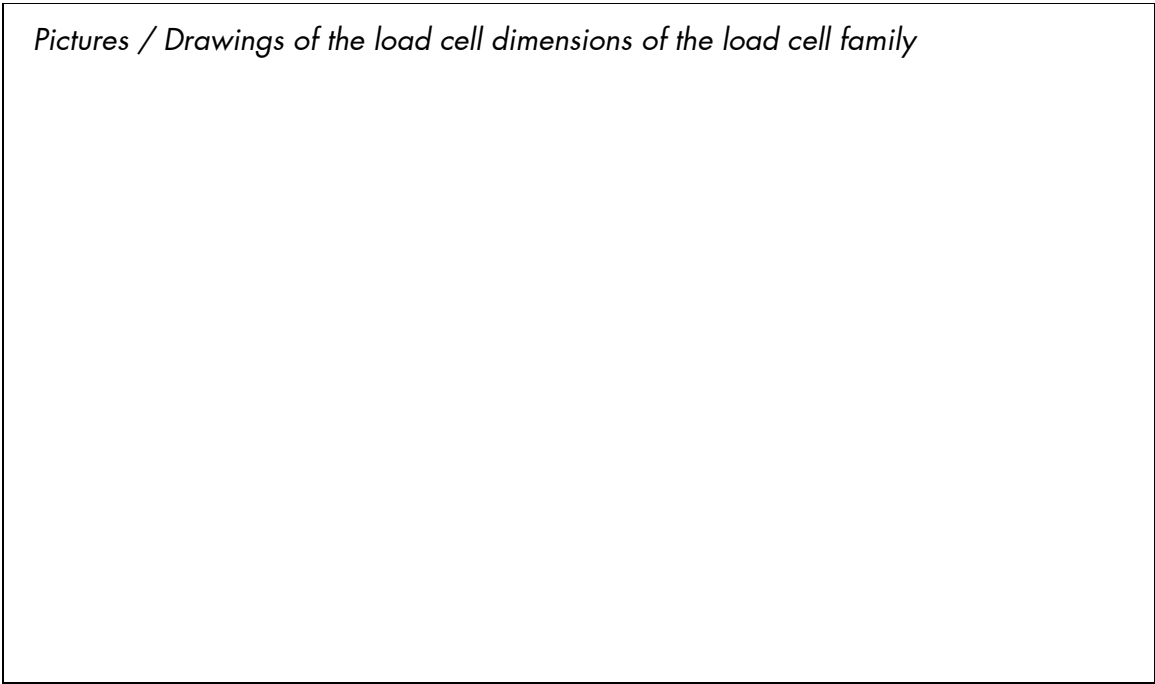

**3.9.11.** Recommended load transmissions of the manufacturer

*Pictures / Drawings of the recommended load transmissions*



**3.9.12.** Results of previous tests that were taken into account

Model designation	Serial number	Justification / Remark	Test Report No. (if available)

### 3.10. Information concerning the test equipment used for the tests

*(including details of simulations and the way uncertainties are taken into account, including the level of "risk." For instance, 95% or  $k=2$ )*

*The following tables have to be completed for each individual piece of test equipment used for the tests.*

#### General information:

For each of the following pieces of test equipment, indicate for which of the following test procedures the test equipment is used:

<i>R60 part 2 reference</i>	<i>Test procedure</i>
8.10.1	<i>Measurement error, repeatability error and temperature effect on minimum dead load output</i>
8.10.2	<i>Determination of creep error</i>
8.10.3	<i>Minimum dead load output return (DR)</i>
8.10.4	<i>Barometric pressure effects (Atmospheric pressure)</i>
8.10.5	<i>Humidity effects for load cells marked with CH or no marked</i>
8.10.6	<i>Humidity effects for load cells marked SH</i>
8.10.7	<i>Additional tests for digital load cells</i>

#### *Example:*

*A test equipment is used for determination the measurement error (R60 part 2: 8.10.1), the creep error (R60 part 2: 8.10.2), the minimum dead load (R60 part 2: 8.10.3) and humidity effect marked with SH (R60 part 2: 8.10.6):*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>	X	X	X				X	



**3.10.1. Force generating system** (if a force generating system or force generating machine is used)

	Description	Remark
Designation		
Type		
Manufacturer		
Identification Number		
Load Range		
Load Steps		
Unit		
Preload		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The force generating system is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

Remarks / picture of the force generating system:

---



---



---



---



---



---



---

**3.10.2. Weights***(if the load cell is tested manually with weights)*

Number / identification	Weight (g, kg, t)	Class <sup>1</sup> / rel. uncertainty (k=2)	Last calibration	Recalibration interval	Certificate No. / report No.

*The Weights are used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

Remarks / picture of the weights:

---



---



---



---



---



---

<sup>1</sup> according to OIML R111

**3.10.3. Temperature chamber (without humidity control)**

	Description	Remark
Designation		
Type		
Manufacturer		
Identification Number		
height x width x length dimension		
Temperature range		
Temperature stability		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The temperature chamber is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

Remarks / picture of the temperature chamber:

---



---



---



---

**3.10.4. Climate chamber (with temperature and humidity control)**

	Description	Remark
Designation		
Type		
Manufacturer		
Identification Number		
height x width x length dimension		
Temperature range		
Temperature stability		
Humidity range		
Humidity stability		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The climate chamber is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

Remarks / picture of the climate chamber:

---



---

---



---



---



---

**3.10.5. Indicator / Indicating instrument**

(for testing analog load cells)

	Description	Remark
Designation		
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

Settings of the indicator / indicating instrument used for the tests

	Description	Remark
Measurement range		
Supply voltage (AC/DC)		
Filter settings		
Cable connections		

*The indicator / indicating instrument is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
-------------------------------------	---------------	---------------	---------------	---------------	---------------	---------------	---------------	---------------

<i>Used for</i>								
-----------------	--	--	--	--	--	--	--	--

Remarks / picture of the indicator / indicating instrument:

---

---

---

---

**4.10.6. Terminal / Digital data processing device**

(for testing digital load cells)

	<b>Description</b>	<b>Remark</b>
Designation		
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

Settings of the indicator / indicating instrument used for the tests

	<b>Description</b>	<b>Remark</b>
Measurement range		
Supply voltage (AC/DC)		
Filter settings		
Cable connections		

*The terminal / digital data processing device is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

Remarks / picture of the terminal / digital data processing device:

---



---



---



---

**3.10.6. Barometric pressure meter**

	Description	Remark
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The barometric pressure meter is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

**3.10.7. Thermometer**

	Description	Remark
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The thermometer is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								



**3.10.8. Moisture analyzer**

	Description	Remark
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The moisture analyzer is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

**3.10.9. Additional test equipment**

*(e.g. burst generator for testing of digital load cells)*

	Description	Remark
Test equipment		
Type		
Manufacturer		
Identification / Serial Number		
Measurement range		
Rel. uncertainty (k=2)		
Last calibration		
Certificate No. / report No.		
Recalibration interval		

*The equipment is used for the following test procedures:*

<i>R60 part 2 reference</i>	<i>8.10.1</i>	<i>8.10.2</i>	<i>8.10.3</i>	<i>8.10.4</i>	<i>8.10.5</i>	<i>8.10.5</i>	<i>8.10.6</i>	<i>8.10.7</i>
<i>Used for</i>								

**3.10.10.** Remarks (settings, pictures, further information)

---

---

---

---

---

---

---

---

---

---

#### 4. Examination

*(To be completed by the Evaluating Authority)*

##### 4.1. Marking requirements (R60 part 1,6.2)

##### 4.1.1. Mandatory markings on the load cell (R60 part 1: 6.2.1)

<i>R60 part 2 reference</i>	<i>Information</i>	<i>Fulfills requirements</i>	
		Yes	No
7.2.1 / 7.2.2	Name or trademark of manufacturer		
7.2.1 / 7.2.2	Manufacturer's own designation or load cell model		
7.2.1	Serial number		
7.2.1 / 7.2.2	Maximum capacity, $E_{\max}$ <sup>1)</sup>		
7.2.1	Year of production		

7.2.1	Type evaluation mark according to R60-2		
-------	---	--	--

<sup>1)</sup> In units of (g, kg, t)

#### 4.1.2. Mandatory markings on the load cell or an accompanying document

(R60 part 1: 6.2.2)

R60 part 1 reference	Mandatory information	On load cell	In document	Fulfills requirements	
				Yes	No
6.2.4.1	Accuracy classes and their symbols				
6.2.4.5	Maximum number of load cell verification intervals, $n_{LC}$				
6.2.4.2	Loading designation (if necessary)				
6.2.4.3	Working temperature designation				
6.2.4.4	Humidity symbol "NH"				
6.2.4.4	Humidity symbol "SH"				
6.2.2	Minimum dead load, $E_{min}$				
6.2.2	Safe load limit, $E_{lim}$				
5.1.3, 6.2.2	Minimum load cell verification interval ( $v_{min}$ )				
6.2.2	Other pertinent conditions				
3.7.2, 5.3.2	Apportionment factor, $p_{LC}$ (if not equal to 0.7)				
5.1.6	Standard classification				
5.1.7	Multiple classifications				

#### 4.1.3. Non-mandatory, additional information (R60-1: 6.2.3)

R60 part 1 reference	Non-mandatory additional information	On load cell	In document	Fulfills requirements	
				Yes	No
5.6.3.1	Humidity symbol "CH"				
3.5.15	Relative $v_{min}$ , Y				
3.5.14	Relative DR, Z				

#### 4.2. Suitability for testing (R60 part 2: 8.3, 8.4)

Date:	Observer:	Serial number:	
			Fulfil requirements
			Yes
Remarks			
Passed <input type="checkbox"/> Yes <input type="checkbox"/> No			

### 4.3. Software (if present) (R60 part 1: 6.1)

Date:	Observer:	Serial number:
Version of software:		Identification code:

	Yes	No
Software protected by sealing		
Automatic change of identification code		
Fixed version number		
Remarks:		

Passed		Yes		No
--------	--	-----	--	----

**4.4. Documentation for type approval (R60 part 1, 8.5)**

	Yes	No	Remarks
a) Description of the general principle of measurement (R60 part 2: 8.5, a)			
b) List and characteristics of essential components + details			
c) Mechanical drawings (R60 part 2: 8.5, b)			
d) Electric/electronic diagrams (R60 part 2: 8.5, c)			
e) Installation requirements (R60 part 2: 8.5, d)			
f) Sealing plan			
g) Panel layout			
h) General information of the software (R60 part 2: 8.5, g)			<i>For details, see R60 part 1, 6.1</i>
i) Operating instructions (R60 part 2: 8.5, e)			
j) Information supporting the manufacturer's assumption (R60 part 2: 8.5, f)			
Other relevant information pertaining to identification of the instrument, diagrams, results of previous tests etc.: (attach photograph(s) and/or outline-drawing(s) here if available):			
Remarks:			

Passed	<input type="checkbox"/>	Yes	<input type="checkbox"/>	No
--------	--------------------------	-----	--------------------------	----

## 5. Performance tests

### 5.1. Results of the Performance tests

Clause R60- parts 1&2	Performance tests	Temperature in °C	report page No.	Maximum error in v	Passed	Failed	remark
5.3 8.10.1	Load cell errors ( $E_L$ ) (see OIML R60-3, No. 2.1.2)						
5.4 8.10.1	Repeatability errors ( $E_R$ ) (see OIML R60-3, No. 2.1.3)						
5.5.1 8.10.2	Creep ( $C_C(t)$ ) (see OIML R60-3, 2.1.5)						
5.5.1 8.10.2	Creep ( $C_C(30-20)$ ) (see OIML R60-3, 2.1.5.2)						

Clause R60- parts 1&2	Performance tests	Temperature in °C	report page No.	Maximum error in v	Passed	Failed	remark
5.5.2 8.10.3	Minimum dead load output return ( $C_{DR}$ ) / (see OIML R60 part 3, 2.1.5.4)						(See note 1) DR=
							(See note 1) DR=
							(See note 1) DR=
							(See note 1) DR=
5.6.3 8.10.5	Humidity effects ( $CH_{min}$ ) / (CH or no mark) (see OIML R60 part 3, 2.1.7.1)						
5.6.3 8.10.5	Humidity effects ( $CH_{max}$ ) / (CH or no mark) (see OIML R60 part 3, 2.1.7.2)						
5.6.3.2	Humidity effects (SH) / (see OIML R60 part 3, 2.1.8)						
5.6.1.3	Temperature effects on minimum dead load output ( $C_M$ ) / (see OIML R60 part 3, 2.1.4)			(See note 2)			
5.6.2	Barometric pressure effects ( $C_P(v_{min})$ ) / (see OIML R60 part 3, 2.1.6)			(See note 2)			

- 1) DR is the minimum dead load output return in units of (g, kg, t) and determined according to OIML R60 part 3, No. 2.1.5.8
- 2) Maximum error in unit  $v_{min}$

Remarks:

---



---



---



---

**5.1.1. Results of the Performance tests for digital load cells**

Clause R60-parts 1&2	Performance tests	Temperature in °C	report page No.	Maximum error in v	Passed	Failed	remark
5.7.2.1 8.10.7.3	Warm-up time / (see OIML R60 part 3, 2.2.1)						
5.7.2.2 8.10.7.4	Power voltage variations / (see OIML R60 part 3, 2.2.2)						
5.7.2.5 8.10.7.5	Short time power reductions / (see OIML R60 part 3, 2.2.3)						
5.7.2.5 8.10.7.6	Bursts (electrical fast transients) (see OIML R60 part 3, 2.2.4)						
5.7.2.5 8.10.7.7	Surge / (see OIML R60 part 3, 2.2.5)						
5.7.2.5 8.10.7.8	Electrostatic discharge / (see OIML R60 part 3, 2.2.6)						
5.7.2.5 8.10.7.9	Electromagnetic susceptibility / (see OIML R60 part 3, 2.2.7)						
5.7.2.5 8.10.7.10	Immunity to conducted electromagnetic fields / (see OIML R60 part 3, 2.2.8)						
5.7.2.6 8.10.7.11	Span stability / (see OIML R60 part 3, 2.2.9)						

Remarks:

---



---



---



---



**5.2. Initial tests and general notes concerning performance tests***(To be completed or under the responsibility of the Evaluating Authority)***5.2.1.Units***Unit (e.g. counts, digits, g, kg, t) in which the measurement result is displayed.*

<i>R60 part 2 reference</i>	<i>Test procedure</i>	<i>Unit</i>
8.10.1	<i>Measurement error, repeatability error and temperature effect on minimum dead load output</i>	
8.10.2	<i>Determination of creep error</i>	
8.10.3	<i>Minimum dead load output return (DR)</i>	
8.10.4	<i>Barometric pressure effects (Atmospheric pressure)</i>	
8.10.5	<i>Humidity effects for load cells marked with CH or no marked</i>	
8.10.6	<i>Humidity effects for load cells marked SH</i>	
8.10.7	<i>Additional tests for digital load cells</i>	

**5.2.2.Measurement range (OIML R60, 5.2, 5.5.2)**

Test procedure (R60 part 2 reference)	$D_{\max}$	$D_{\min}$	Conversion factor f [indication / v] (see OIML R60-3, 2.1.2.4)	Fulfills requirements	
				yes	no
8.10.1					
8.10.2					
8.10.3					
8.10.4					
8.10.5					
8.10.6					
8.10.7					

Passed

☐ Yes☐ No



**5.2.3. Conditions**

(see OIML R60 part 2, 8.8.1)

*(To ensure that these requirements are met, the calculations should be carried out using lower  $n$  values than the  $n_{LC}$  specified. The calculations made do not include the application of 8.8.1.)*

Check that

$$V_{\min} \leq \frac{D_{\max} - D_{\min}}{n}.$$

It should be sufficient to carry out the calculations with  $n = n_{LC}$ ,  $n_{\max} - 500$  and  $n = n_{LC} - 1\,000$  if applicable.

Test procedure (R60 part 2 Reference)	$D_{\min}$	$D_{\max}$	$n_{LC}$	Is the requirement $v_{\min} \leq \frac{D_{\max} - D_{\min}}{n}$ fulfilled with					
				$n_{LC}$		$n_{LC} - 500$		$n_{LC} - 1000$	
				Yes	No	Yes	No	Yes	No
8.10.1									
8.10.2									
8.10.3									
8.10.4									
8.10.5									
8.10.6									
8.10.7									

Passed

☐ Yes☐ No**5.2.4. Input impedance**

Measure the input impedance and compare the result with the input impedance in OIML R60-3, 4.5

Input impedance		Fulfills the requirements	
Manufacturer specification According to OIML R60 part 3, 4.1.1	Measured value	yes	no

### 5.3. Load test data (Load cell error $E_L$ ) 3 runs

Ref.: R60 part 2, 8.10.1.1 to 8.10.1.11. Complete one sheet for each test temperature, one for each humidity (SH) test in 8.10.6, and when applicable, one for each electronics power voltage in 8.10.7.4.

Application no.:	_____				
Load cell model:	_____				
Serial no.:	_____				
$E_{max}$ :	_____				
$n_{LC}$ :	_____				
$V_{min}$ :	_____				
$p_{LC}$ :	_____	DR:	_____		
Force-generating system:	_____				
Indicating instrument:	_____				
Evaluator:	_____				

Date:					
Temperature:					°C
Relative humidity:					%
Barometric pressure:					kPa
Indicator temperature:					°C

Electronics power voltage					
(when applicable):	_____	V			

**Table 6.3** (3 runs)

[illegible]

Notes: 1) \* = Average initial minimum test load indication.  
2) Absolute (not relative) time shall be recorded.

**5.4. Load test data (Load cell error  $E_L$ ) 5 runs**

R60 part 2 Ref.: 8.10.1.1 to 8.10.1.11. Complete one sheet for each test temperature, one for each humidity (SH) test in 8.10.6, and when applicable, one for each electronics power voltage in 8.10.7.4.

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_ $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Evaluator: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

	At start	At end	
Date:			
Temperature:			°C
Relative humidity:			%
Barometric Pressure:			kPa
Indicator temperature:			°C

Electronics power voltage (when applicable): \_\_\_\_\_ V

**Table 6.4** (5 runs)

[illegible]

Notes: 1) \* = Average initial minimum test load indication.

2) Absolute (not relative) time shall be recorded.

### 5.5. Load cell errors ( $E_L$ ) calculation

R60 parts 1&2 Ref: 5.3.1; 8.10.1.12 to 8.10.1.14  
R60 part 3: 2.1.2.2

Application no.: _____ Load cell model: _____ Serial no.: _____ $E_{max}$ : _____ $n_{LC}$ : _____ $V_{min}$ : _____ $p_{LC}$ : _____ DR: _____ Force-generating system: _____ Indicating instrument: _____ Evaluator: _____	<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 50%;"></th> <th style="width: 25%;">At start</th> <th style="width: 25%;">At end</th> </tr> </thead> <tbody> <tr> <td>Date:</td> <td></td> <td></td> </tr> <tr> <td>Temperature:</td> <td></td> <td></td> </tr> <tr> <td>Relative humidity:</td> <td></td> <td></td> </tr> <tr> <td>Barometric pressure:</td> <td></td> <td></td> </tr> <tr> <td>Indicator temperature:</td> <td></td> <td></td> </tr> </tbody> </table> <div style="text-align: right; margin-top: -20px;">             °C % kPa °C           </div> Conversion factor, f: _____  75% test load (g, kg, or t): _____ Reference indication at 75% test load: _____		At start	At end	Date:			Temperature:			Relative humidity:			Barometric pressure:			Indicator temperature:		
	At start	At end																	
Date:																			
Temperature:																			
Relative humidity:																			
Barometric pressure:																			
Indicator temperature:																			

Table 6.5

[illegible]

Minimum test load,  $D_{\min}$ : \_\_\_\_\_ PASS: ☐ FAIL: ☐

- Notes:*
- 1 Load/reference indications: if a 75 % load point was not obtained, a straight line interpolation between the adjacent higher and lower load point indications is used (see 5.3.1 and calculation procedures in 2.1.2.2).
  - 2 Error,  $E_L$ : the difference between the test indication and the reference indication divided by the conversion factor,  $f$ .
  - 3 Test load values are values above minimum test load,  $D_{min}$ .



**5.6. Repeatability errors ( $E_R$ ) calculation**

R60 parts 1&amp;2 Ref.: 5.4; 8.10.1.15

R60 part 3: 2.1.3.

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_ Force-generating system: \_\_\_\_\_

Serial no.: \_\_\_\_\_ Indicating instrument: \_\_\_\_\_

 $E_{max}$ : \_\_\_\_\_ Evaluator: \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_ Conversion factor,  $f$ : \_\_\_\_\_ $V_{min}$ : \_\_\_\_\_ $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_**Table 6.6**

Test load (unit)	.... °C (20 °C)		.... °C ( $T_1$ °C)		.... °C ( $T_2$ °C)		.... °C (20 °C)		MPE ( $\nu$ )
	Repeatability error (counts)	Repeatability error ( $\nu$ )	Repeatability error (counts)	Repeatability error ( $\nu$ )	Repeatability error (counts)	Repeatability error ( $\nu$ )	Repeatability error (counts)	Repeatability error ( $\nu$ )	

PASS: ☐ FAIL: ☐

**Note:** Error,  $E_R$ : the maximum difference between the three test indications divided by the conversion factor,  $f$  (classes C and D) or the maximum difference between the five test indications divided by the conversion factor,  $f$  (classes A and B).

### 5.7. Temperature effects on minimum dead load output return (MDLO)

R60 parts 1&2 Ref.: 5.5.2; 8.10.1.16;  
R60 part 3: 2.1.4.

Application no.: \_\_\_\_\_ Force-generating system: \_\_\_\_\_  
Load cell model: \_\_\_\_\_ Indicating instrument: \_\_\_\_\_  
Serial no.: \_\_\_\_\_ Evaluator: \_\_\_\_\_  
 $E_{\max}$ : \_\_\_\_\_  
 $n_{LC}$ : \_\_\_\_\_  
 $v_{\min}$ : \_\_\_\_\_ Conversion factor, f: \_\_\_\_\_  
 $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_

**Table 6.7.**

Temperature °C	Indication ( )	Change ( $C_M$ ) (v)	Change ( $v_{\min} / \dots \text{°C}$ )	mpc ( $v_{\min} / \dots \text{°C}$ )
				$p_{LC}$
				$p_{LC}$
				$p_{LC}$

PASS: ☐ FAIL: ☐

- Notes:*
- 1 MDLO: minimum dead load output.
  - 2 Indication: the average initial minimum test load indication obtained from Table D.1.
  - 3 The maximum permissible change (mpc) allowed is: ( $v_{\min} / 5 \text{ °C}$ ) for classes B, C, and D; ( $v_{\min} / 2 \text{ °C}$ ) for class A.
  - 4 Change,  $C_M$  (v): the difference between the observed indications, and the indications at the prior temperature, divided by the conversion factor, f.

R60 parts 1&2 Ref: 5.5.1, 5.5.2; 8.10.2, 8.10.3. Complete one sheet for each test temperature.

	At start	At end	
Date:			
Temperature:			°C
Relative humidity:			%
Barometric pressure:			kPa
Indicator temperature:			°C

Conversion factor,  $f$ : \_\_\_\_\_

**Table 6.8**[illegible]

DR (v):	<input type="text"/>	30 minute creep: PASS: <input type="checkbox"/> FAIL: <input type="checkbox"/>
actual time (s):	<input type="text"/>	20 – 30 minute creep difference (< 0.15*MPE): PASS: <input type="checkbox"/> FAIL: <input type="checkbox"/>
specified time (s):	<input type="text"/>	DR < 0.5 v: PASS: <input type="checkbox"/> FAIL: <input type="checkbox"/>
MPE for DR (v):	<input type="text"/>	DR within manuf. Specified DR requirements: PASS: <input type="checkbox"/> FAIL: <input type="checkbox"/>

- Notes:*
- 1 Change (v) for creep: the observed indication minus the initial "load" indication (\*\*) divided by the conversion factor, f.
  - 2 Determine the difference between the reading obtained at 20 minutes and the reading obtained at 30 minutes (see 5.5.1).
  - 3 Change (v) for DR: the initial indication (\*\*\*) minus the initial "no load" indication (\*) divided by the conversion factor, f.
  - 4 Absolute (not relative) time shall be recorded.

## 5.9. Barometric pressure effects (C<sub>P</sub>)

R60 parts 1&2 Ref: 5.6.2; 8.7.3.7; 8.10.4

R60 part 3: 2.1.6.

Complete one sheet for each test temperature.

Application no.: _____			
Load cell model: _____			
Serial no.: _____			
E <sub>max</sub> : _____ E <sub>min</sub> : _____			
n <sub>LC</sub> : _____ p <sub>LC</sub> : _____			
Y: _____ Z: _____			
v <sub>min</sub> : _____ DR: _____			
Force-generating system: _____			
Test load, D <sub>max</sub> : _____ D <sub>min</sub> : _____			
Indicating instrument: _____			
Evaluator: _____			

	At start	At end	
Date:			
Temperature:			°C
Relative humidity:			%
Barometric pressure:			hPa
Indicator temperature:			°C

Conversion factor, f: \_\_\_\_\_

Table 6.9

Pressure (hPa)	Indication (counts)	Time hh:mm	Change (v)	Change (v <sub>min</sub> / kPa)	mpc (vmin / kPa)
			0	0	0
					1
					1
					1

PASS: ☐ FAIL: ☐

**5.10. Humidity effects****5.10.1. Humidity effects (CH or no mark)**

R60 parts 1&amp;2 Ref: 5.6.3; 8.7.3.8; 8.10.5

R60 part 3: 2.1.7

**Form 6.10.1.(a): Humidity effects summary (CH or no mark)**

Application no.: \_\_\_\_\_  
 Load cell model: \_\_\_\_\_  
 Serial no.: \_\_\_\_\_  
 $E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_  
 $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_  
 Y: \_\_\_\_\_ Z: \_\_\_\_\_  
 $v_{\min}$ : \_\_\_\_\_ DR: \_\_\_\_\_  
 Force-generating system: \_\_\_\_\_  
 Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_  
 Indicating instrument: \_\_\_\_\_  
 Evaluator: \_\_\_\_\_

	<i>At start</i>	<i>At end</i>	
<i>Date:</i>			
<i>Temperature:</i>			°C
<i>Relative humidity:</i>			%
<i>Barometric pressure:</i>			hPa
<i>Indicator temperature:</i>			°C

Conversion factor,  $f$ : \_\_\_\_\_

Table 6.10.1.(a)

Test load (g, kg, or t)	Before humidity test		After humidity test		Change (v)	mpc (v)
	Indication (counts)	Time (hh mm ss)	Indication (counts)	Time (hh mm ss)		
Average indication at $D_{min}$ (a) $C_{Hmin} =$						
Average indication at $D_{max}$ (‡)						
Average difference (*) $C_{Hmax} =$						1

← < 4%  $n_{LC}$ (a) Indications at minimum test load Change (a),  $C_{Hmin}$ : PASS: ☐ FAIL: ☐

(‡) Indications at maximum test load (see note 3)

(\*) Average, see 6.6.3 and OIML R60-3, 2.1-7 Change (\*),  $C_{Hmax}$ : PASS: ☐ FAIL: ☐

## Notes:

- 1 This test is not necessary if the load cell is marked NH or SH.
- 2 Change (v): the difference between the indication after and before humidity exposure divided by the conversion factor, f.
- 3 Use five test runs for Class A and B; use 3 test runs for Class C and D.
- 4 Absolute (not relative) time shall be recorded.
- 5 For family certification this test is not necessary, if a pattern with a smaller capacity and the same or better metrological characteristics has passed this test.

**Form 6.10.1.(b): Load test data (EL) - 3 runs**

R60 part 2 Ref.: 8.10.1.1 to 8.10.1.11. Complete this form if the measurement error is determined **before** the humidity test (CH) is carried out (not mandatory)

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_

Y: \_\_\_\_\_ Z: \_\_\_\_\_

 $v_{\min}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_

	<i>At start</i>	<i>At end</i>	
<i>Date:</i>			
<i>Temperature:</i>			°C
<i>Relative humidity:</i>			%
<i>Barometric pressure:</i>			hPa
<i>Indicator temperature:</i>			°C

*Electronics power voltage**(when applicable):* \_\_\_\_\_

[illegible]

64



**Form 6.10.1.(c): Load test data (EL) - 3 runs**

R60 part 2 Ref.: 8.10.1.1 to 8.10.1.11. Complete this form if the measurement error is determined **after** the humidity test (CH) is carried out (not mandatory)

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_

Y: \_\_\_\_\_ Z: \_\_\_\_\_

 $v_{\min}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_

	<i>At start</i>	<i>At end</i>	
<i>Date:</i>			
<i>Temperature:</i>			°C
<i>Relative humidity:</i>			%
<i>Barometric pressure:</i>			hPa
<i>Indicator temperature:</i>			°C

*Electronics power voltage**(when applicable):* \_\_\_\_\_

[illegible]

66

**Form 6.10.1(d): Load test data ( $E_L$ ) - 5 runs**

R60 part 2 Ref.: 8.10.1.1 to 8.10.1.11. Complete this form if the measurement error is determined **before** the humidity test (CH) is carried out (not mandatory)

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_

Y: \_\_\_\_\_ Z: \_\_\_\_\_

 $v_{\min}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_

	<i>At start</i>	<i>At end</i>	
<i>Date:</i>			
<i>Temperature:</i>			°C
<i>Relative humidity:</i>			%
<i>Barometric pressure:</i>			hPa
<i>Indicator temperature:</i>			°C

*Electronics power voltage*  
*(when applicable):* \_\_\_\_\_

**Table 6.10.1.(d) 5 runs**

[illegible]

Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_


Notes: \*Average initial minimum test load indication

**Form 6.10.1(e): Load test data ( $E_L$ ) - 5 runs**R60 part 2 Ref.: 8.10.1.1 to 8.10.1.11. Complete this form if the measurement error is determined **after** the humidity test (CH) is carried out (not mandatory)

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_

Y: \_\_\_\_\_ Z: \_\_\_\_\_

 $v_{\min}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_

	At start	At end	
Date:			
Temperature:			°C
Relative humidity:			%
Barometric pressure:			hPa
Indicator temperature:			°C

Electronics power voltage  
(when applicable): \_\_\_\_\_

**Table 6.10.1.(e) 5 runs**

[illegible]


Notes:    *\*Average initial minimum test load indication*

### **Form 6.10.2. Humidity effects (SH) summary**

Conversion factor, f: \_\_\_\_\_  
 Page of load test before humidity test: \_\_\_\_\_  
 Page of load test during humidity test: \_\_\_\_\_  
 Page of load test after humidity test: \_\_\_\_\_

**Table 6.10.2**[illegible]



PASS: ☐FAIL: ☐*Notes:*

1. Load/Reference indications: if at 75% load point was not obtained, a straight line interpolation between the adjacent higher and lower load point indication is used.
2. Error,  $E_L$ : the difference between the test reference and the reference indication divided by the conversion factor,  $f$ .
3. Test load values are values above minimum test load,  $D_{min}$ .
4. Conditioning period: the time period for exercising the load cell.
5. For family certification this test is not necessary, if a pattern with a smaller capacity and the same or better metrological characteristics has passed this test.

**5.11. Warm-up time****Form 6.11 Warm-up time**

R60 parts 1&amp;2 Ref.: 3.5.17; 8.10.7.3

R60 part 3: 2.2.1

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{max}$ : \_\_\_\_\_  $E_{min}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_

Y: \_\_\_\_\_ Z: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{max}$ : \_\_\_\_\_  $D_{min}$ : \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_ Conversion factor,  $f$ : \_\_\_\_\_ counts/v

Duration of disconnection before test: \_\_\_\_\_

	At start	At end
Date:		
Time:		
Temperature:		°C
Relative humidity:		%
Barometric pressure:		hPa

**Table 6.11**

Test load (units)	Preloads	
	Indication (counts)	Time hh:mm:ss
D <sub>min</sub>		
D <sub>max</sub>		
D <sub>min</sub>		
D <sub>max</sub>		
D <sub>min</sub>		
D <sub>max</sub>		

		Initial run		After 5 min.		After 15 min.		After 30 min.		mpc v
		Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	
	D <sub>min</sub>									
	D <sub>max</sub>									
Span	Counts									
Span	v									
Change	v									

PASS: ☐ FAIL: ☐

Notes:

1. Absolute (not relative) time shall be recorded.
2. Span: the result of subtraction of the indication at minimum test load from the indication at maximum test load. All span errors (error at maximum test load minus the error at minimum test load) shall be within the maximum permissible error during the 30 minute test.
3. The change of span must not exceed v<sub>min</sub>.
4. Change: the difference between the span and the initial run span.
5. Maximum permissible change, mpc: the absolute value of the maximum permissible error for the maximum test load applied.
6. Exercises have to be run before disconnection.

## 5.12. Power Voltage Variation

### Form 6.12 Power Voltage Variation

R60 parts 1&2 Ref.: 5.7.2.2; 5.7.2.3; 5.7.2.4; 8.10.7.4.  
R60 part 3: 2.2.2

Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

Application no.: \_\_\_\_\_ Date: \_\_\_\_\_

Load cell model: \_\_\_\_\_ Time: \_\_\_\_\_

Serial no.: \_\_\_\_\_ Temperature: \_\_\_\_\_ °C

$E_{\max}$ : \_\_\_\_\_  $E_{\min}$ : \_\_\_\_\_ Relative humidity: \_\_\_\_\_ %

$n_{LC}$ : \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_ Barometric pressure: \_\_\_\_\_ hPa

Y: \_\_\_\_\_ Z: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Test load,  $D_{\max}$ : \_\_\_\_\_  $D_{\min}$ : \_\_\_\_\_ Conversion factor,  $f$ : \_\_\_\_\_ counts/v

Indicating instrument: \_\_\_\_\_ Main voltage: \_\_\_\_\_

Evaluator: \_\_\_\_\_ AC: ☐ DC: ☐

At start

At end

Table 6.12 (a)

Test load (units)	Preloads	
	Indication (counts)	Time hh:mm:ss
$D_{\min}$		
$D_{\max}$		
$D_{\min}$		
$D_{\max}$		
$D_{\min}$		
$D_{\max}$		

Notes: 1) Reference indications: if at 75% load point was not obtained, a straight line interpolation between the adjacent higher and lower indication is used. (see 9.8.2 and calculation procedures in OIML R60-3, 2.1.2)

2) Error: the difference between the test indication and the reference indication divided by the conversion factor,  $f$ .

3) The change of span must not exceed  $v_{\min}$ .

4) When a voltage range is marked, use the average value as the reference value and determine upper and lower values of applied voltage according to A.4.7.3.

5) Upper limit not applicable to battery powered load cells

6) At lower limit, battery powered load cells shall function and be within MPE, or cease to function

		Initial run with main voltage		lower limit main voltage – 15%		upper limit main voltage + 15%		mpc v
		Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	
	$D_{\min}$							
	$D_{\max}$							
Span	Counts							
Span	v							
Change	v							

PASS: ☐FAIL: ☐

If AC power supply is used (not applicable for battery power supply)

Table 6.12 (b)

		Initial run with main voltage		lower limit frequency – 2%		upper limit frequency + 2%		mpc v
		Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	Indication (counts)	Time hh:mm:ss	
D <sub>min</sub>								
D <sub>max</sub>								
Span	Counts							
Span	v							
Change	v							

PASS: ☐FAIL: ☐

### 5.13. Short time power reductions

#### Form 6.13 Short time power reductions

R60 parts 1&amp;2 Ref: 5.7.2.5, 8.10.7.5.

R60 part 3: 2.2.3

Application no.: \_\_\_\_\_  
 Load cell model: \_\_\_\_\_  
 Serial no.: \_\_\_\_\_  
 E<sub>max</sub>: \_\_\_\_\_  
 n<sub>LC</sub>: \_\_\_\_\_  
 v<sub>min</sub>: \_\_\_\_\_  
 p<sub>LC</sub>: \_\_\_\_\_  
 DR: \_\_\_\_\_  
 Force-generating system: \_\_\_\_\_  
 Indicating instrument: \_\_\_\_\_  
 Evaluator: \_\_\_\_\_

Date: \_\_\_\_\_  
 Time: \_\_\_\_\_  
 Temperature: \_\_\_\_\_ °C  
 Relative humidity: \_\_\_\_\_ %  
 Barometric pressure: \_\_\_\_\_ kPa  
 Conversion factor, f: \_\_\_\_\_  
 Minimum test load, D<sub>min</sub>: \_\_\_\_\_  
 Reference voltage range: \_\_\_\_\_ V

Table 6.13

Test load (g, kg, or t)	Disturbance				Result			
	Amplitude (%)	Duration (cycles)	Number of disturbances	Repetition interval (v)	Indication (     )	Difference (v)	Significant fault > v <sub>min</sub>	
							No	Yes (remarks)
Without disturbance								
	0	0.5	10					
	50	1	10					

Equipment used (supply sketch if necessary):

PASS: ☐FAIL: ☐

Remarks:

*Note:* In the case of a voltage range, use the average value as the reference value.

**5.14. Burst (electrical fast transients)****Form 6.14.1 Burst (electrical fast transients) – power supply lines**

R60 parts 1&amp;2 Ref: 8.10.7.6, 5.7.2.5

R60 part 3: 2.2.4

Application no.: _____	Date: _____
Load cell model: _____	Time: _____
Serial no.: _____	Temperature: _____ °C
$E_{\max}$ : _____	Relative humidity: _____ %
$n_{LC}$ : _____	Barometric pressure: _____ kPa
$v_{\min}$ : _____	
$p_{LC}$ : _____ DR: _____	
Force-generating system: _____	Conversion factor, $f$ : _____
Indicating instrument: _____	Minimum test load, $D_{\min}$ : _____
Evaluator: _____	

**Table 6.14.1**

Power supply lines: test voltage = 1 kV; duration of test = 1 minute at each polarity

Test load (g, kg, or t)	Connection			Polarity	Result			
	L to ground	N to ground	PE to ground		Indication (        )	Difference (v)	Significant fault > v <sub>min</sub>	
							No	Yes (remarks)
	without disturbance							
	X			pos				
				neg				
	without disturbance							
		X		pos				
				neg				
	without disturbance							
			X	pos				
				neg				

L = phase, N = neutral, PE = protective earth

PASS: ☐FAIL: ☐

Equipment used (supply sketch if necessary)

**Form 6.14.2 Burst (electrical fast transients) – I/O circuits and communications lines**

R60 parts 1&amp;2 Ref: 8.10.7.6, 5.7.2.5

R60 part 3: 2.2.4

Application no.: _____	Date: _____
Load cell model: _____	Time: _____
Serial no.: _____	Temperature: _____ °C
$E_{\max}$ : _____	Relative humidity: _____ %
$n_{LC}$ : _____	Barometric pressure: _____ kPa
$v_{\min}$ : _____	
$p_{LC}$ : _____ DR: _____	
Force-generating system: _____	Conversion factor, $f$ : _____
Indicating instrument: _____	Minimum test load, $D_{\min}$ : _____
Evaluator: _____	

**Table 6.14.2**

Test load (g, kg, or t)	Cable interface	Polarity	Result			
			Indication ( )	Difference (v)	Significant fault > v <sub>min</sub>	
					No	Yes (remarks)
	without disturbance					
		pos				
		neg				
	without disturbance					
		pos				
		neg				
	without disturbance					
		pos				
		neg				
	without disturbance					
		pos				
		neg				
	without disturbance					
		pos				
		neg				
	without disturbance					
		pos				
		neg				

Equipment used (supply sketch if necessary)

PASS: ☐FAIL: ☐

Remarks:

*Note:* Explain or make a sketch indicating where the clamp is located on the cable: if necessary use additional page(s).

**5.15. Surge****Form 6.15 Surge**

R60 parts 1&amp;2 Ref: 8.10.7.7, 5.7.2.5

R60 part 3: 2.2.5

Application no.:	_____	Date:	
Load cell model:	_____	Time:	
Serial no.:	_____	Temperature:	°C
$E_{\max}$ :	_____	Relative humidity:	%
$n_{LC}$ :	_____	Barometric pressure:	kPa
$v_{\min}$ :	_____		
$p_{LC}$ :	_____ DR: _____	Conversion factor, $f$ :	_____
Force-generating system:	_____	Minimum test load, $D_{\min}$ :	_____
Indicating instrument:	_____		
Evaluator:	_____		

Table 6.15

<b>OIML R 60-2,</b> .....  [unit] <input type="checkbox"/> [g]; <input type="checkbox"/> [kg]; <input type="checkbox"/> [t]	Test conditions Surges on signal, data and control lines				Observer's name:		
	Output gained	<input type="checkbox"/>	using actual loads		Line to line 1 kV		
			Test load:		Line to earth 2 kV		
		<input type="checkbox"/>	simulating loading				
			using:				
	Cable:				<input type="checkbox"/> Symmetrical line		
	Date:		Start	Stop	<input type="checkbox"/> Unsymmetrical line		
	Time:				Specimen:		
	Ambient temperature		°C	°C	$f$		
	Relative humidity		%	%	$D_{min}$ [unit]		
Barometric Pressure		kPa	kPa	$D_{max}$ [unit]			
	Cycle phase	Initial	During exposure		After		
	Load						
Time	Start						
	Stop						
Quantity [unit]	reference						
	indicated						
Error [ $v_{min}$ ]							
relative error [%] $E_{ii}$							
MPE [%]							
	Pass	<input type="checkbox"/>			<input type="checkbox"/>		
	Fail	<input type="checkbox"/>			<input type="checkbox"/>		
<b>Observed faults after exposure</b>							
Fault limit [%]		.....					
Line to line (N/A for balanced)		Fault/Deviation		Significant		Acts on fault	
$\uparrow \blacksquare$	$\downarrow \blacksquare$			Yes	No	Yes	No
3x				<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
	3x			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Line to earth							
3x				<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
	3x			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Observations							
Result			Pass	<input type="checkbox"/>	Fail	<input type="checkbox"/>	



**5.16. Electrostatic discharge****Form 6.16.1 Electrostatic discharge – direct application**

R60 parts 1&amp;2 Ref: 8.10.7.8, 5.7.2.5

R60 part 3: 2.2.6

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

 $E_{\max}$ : \_\_\_\_\_ $n_{LC}$ : \_\_\_\_\_ $v_{\min}$ : \_\_\_\_\_ $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

Evaluator: \_\_\_\_\_

Date: \_\_\_\_\_

Time: \_\_\_\_\_

Temperature: \_\_\_\_\_ °C

Relative humidity: \_\_\_\_\_ %

Barometric pressure: \_\_\_\_\_ kPa

Conversion factor,  $f$ : \_\_\_\_\_Minimum test load,  $D_{\min}$ : \_\_\_\_\_☐ Contact discharges☐ Paint penetration☐ Air discharges

Polarity (see Note 2):

☐ Positive☐ Negative**Table 6.16.1**

Test load (g, kg, or t)				Result			
	Test voltage (kV)	No. of discharges ≥ 10	Repetition interval (s)	Indication (       )	Difference (v)	Significant fault > v <sub>min</sub>	
						No	Yes (remarks)
	without disturbance						
	2						
	4						
	8 (air discharges)						

PASS: ☐ FAIL: ☐

Remarks:

- Notes: 1 If the load cell fails, the test point at which this occurs shall be recorded.  
 2 IEC Publication 61000-4-2 (1999-05) Ed 1.1 Consolidated edition specifies that the test be conducted with the most sensitive polarity.

**Form 6.16.2 Electrostatic discharge – indirect application**

R60 parts 1&amp;2 Ref: 8.10.7.8, 5.7.2.5

R60 part 3: 2.2.6

Application no.: \_\_\_\_\_  
 Load cell model: \_\_\_\_\_  
 Serial no.: \_\_\_\_\_  
 $E_{\max}$ : \_\_\_\_\_  
 $n_{LC}$ : \_\_\_\_\_  
 $v_{\min}$ : \_\_\_\_\_  
 $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_  
 Force-generating system: \_\_\_\_\_  
 Indicating instrument: \_\_\_\_\_  
 Evaluator: \_\_\_\_\_

Date: \_\_\_\_\_  
 Time: \_\_\_\_\_  
 Temperature: \_\_\_\_\_ °C  
 Relative humidity: \_\_\_\_\_ %  
 Barometric pressure: \_\_\_\_\_ kPa  
 Conversion factor,  $f$ : \_\_\_\_\_  
 Minimum test load,  $D_{\min}$ : \_\_\_\_\_

Polarity (see Note 2):

☐

Positive

☐

Negative

**Table 6.16.2.1 – Horizontal coupling plane**

Test load (g, kg, or t)				Result			
	Test voltage (kV)	No. of discharges ≥ 10	Repetition interval (s)	Indication (        )	Difference (v)	Significant fault > v <sub>min</sub>	
						No	Yes (remarks)
	without disturbance						
	2						
	4						
	6						

**Table 6.16.2.2 – Vertical coupling plane**

Test load (g, kg, or t)				Result			
	Test voltage (kV)	No. of discharges ≥ 10	Repetition interval (s)	Indication (            )	Difference (v)	Significant fault > v <sub>min</sub>	
						No	Yes (remarks)
	without disturbance						
	2						
	4						
	6						

PASS: ☐FAIL: ☐

Remarks:

- Notes:
- 1 If the load cell fails, the test point at which this occurs shall be recorded.
  - 2 IEC Publication 61000-4-2 (1999-05) Ed 1.1 Consolidated edition specifies that the test be conducted with the most sensitive polarity.



**Form 6.16.3 Electronic discharge (continued) – specification of test points**

R60 parts 1&amp;2 Ref.: 8.10.7.8, 5.7.2.5

R60 part 3: 2.2.6

Specify test points utilized on load cell and test equipment used, e.g., by photos or sketches.

## a) Direct application

Contact discharges:

Air discharges:

## b) Indirect application

**6.17. Electromagnetic susceptibility****Form 6.17.1 Electromagnetic susceptibility**

R60 parts 1&amp;2 Ref.: 8.10.7.9, 5.7.2.5

R60 part 3: 2.2.7

Application no.: _____	Date: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	
Load cell model: _____	Time: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	
Serial no.: _____	Temperature: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	°C
$E_{\max}$ : _____	Relative humidity: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	%
$n_{LC}$ : _____	Barometric pressure: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	kPa
$v_{\min}$ : _____		
$p_{LC}$ : _____ DR: _____		
Force-generating system: _____	Conversion factor, $f$ : _____	
Indicating instrument: _____	Minimum test load, $D_{\min}$ : _____	
Evaluator: _____		

Rate of sweep:



Test load:



Test load material:

**Table 6.17**

Disturbance				Result			
Antenna	Frequency range (MHz <sub>z</sub> )	Polarization	Facing load cell	Indication ( )	Difference (v)	Significant fault > v <sub>min</sub>	
						No	Yes (remarks)
without disturbance							
		Vertical	Front				
			Right				
			Left				
			Rear				
		Horizontal	Front				
			Right				
			Left				
			Rear				

PASS: ☐FAIL: ☐

Frequency range: 26 – 1 000 MHz

Field strength: 3 V/m

Modulation: 80% AM, 1 kHz sine wave

Remarks:

*Note:* If the load cell fails, the test point at which this occurs shall be recorded.

**Form 6.17.2 Electromagnetic susceptibility (continued) – description of the test set-up**

Describe the set-up of the test and equipment, e.g., by photos or sketches:

## 6.18. Immunity to conducted electromagnetic fields

R60 parts 1&2 Ref.: 8.10.7.10, 5.7.2.5

R60 part 3: 2.2.8

### Form 6.18 Immunity to conducted electromagnetic fields

Application no.: _____	Date: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	
Load cell model: _____	Time: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	
Serial no.: _____	Temperature: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	°C
$E_{\max}$ : _____	Relative humidity: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	%
$n_{LC}$ : _____	Barometric pressure: <table border="1" style="display: inline-table; width: 150px; height: 25px;"></table>	kPa
$v_{\min}$ : _____		
$p_{LC}$ : _____ DR: _____		
Force-generating system: _____	Conversion factor, $f$ : _____	
Indicating instrument: _____	Minimum test load, $D_{\min}$ : _____	
Evaluator: _____		

Rate of sweep:	<table border="1" style="display: inline-table; width: 120px; height: 25px;"></table>	
Test load:	<table border="1" style="display: inline-table; width: 120px; height: 25px;"></table>	Test load material: <table border="1" style="display: inline-table; width: 120px; height: 25px;"></table>

<b>OIML R 60-2,</b> .....  <b>[unit]</b> <input type="checkbox"/> [g]; <input type="checkbox"/> [kg]; <input type="checkbox"/> [t]	Test conditions RF current injection				Observer's name:	
	Output gained	<input type="checkbox"/>	using actual loads			
			Test load:		$f_i =$ _____ MHz	
		<input type="checkbox"/>	simulating loading		$f_h =$ _____ MHz	
			using:		RF voltage $V_{emf}$	
	Cable exposed				Modulation % AM	
	Date:		Start	Stop	Dwell time _____ s	
	Time:				Specimen:	
	Ambient temperature		°C	°C	$f$	
	Relative humidity		%	%	$D_{min}$ [unit]	
Barometric Pressure		kPa	kPa	$D_{max}$ [unit]		
<b>Frequency cycle</b>	Cycle phase	<b>Initial</b>	<b>During exposure</b>	<b>After</b>		
	Load					
Time	Start					
	Stop					
Quantity [unit]	reference					
	indicated					
Error [ $v_{min}$ ]						
relative error [%] $E_i$						
MPE [%]						
	Pass	<input type="checkbox"/>		<input type="checkbox"/>		
	Fail	<input type="checkbox"/>		<input type="checkbox"/>		
<b>Observed faults during exposure</b>						
Fault limit [%]		.....				
Frequency		Fault/Deviation	Significant		Acts on fault	
MHz			Yes	No	Yes	No
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
			<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Observations						
Result		Pass	<input type="checkbox"/>	Fail	<input type="checkbox"/>	

## 6.19. Span Stability

### Form 6.19.1 (3 runs) Span stability – measurement data for classes C and D

R60 parts 1&amp;2 Ref.: 8.10.7.11, 5.7.2.6

R60 part 3: 2.2.9

Application no.: \_\_\_\_\_ Force-generating system: \_\_\_\_\_ Notes: \_\_\_\_\_  
 Load cell model: \_\_\_\_\_ Indicating instrument: \_\_\_\_\_ *I* Span is the result of subtracting the  
 Serial no.: \_\_\_\_\_  $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_ average indication at minimum test load  
 $E_{max}$ : \_\_\_\_\_ Conversion factor, f: \_\_\_\_\_ from the average indication at maximum test  
 $n_{LC}$ : \_\_\_\_\_ Minimum test load,  $D_{min}$ : \_\_\_\_\_ Load.  
 $V_{min}$ : \_\_\_\_\_ Maximum test load,  $D_{max}$ : \_\_\_\_\_ 2 Absolute (not relative) time shall be  
 recorded.

**Table 6.19.1. (3 runs)**

#### Measurement no. 1:

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_ Remarks: \_\_\_\_\_

Date: \_\_\_\_\_  
 Time: \_\_\_\_\_  
 Temperature: \_\_\_\_\_ °C  
 Relative humidity: \_\_\_\_\_ %  
 Barometric pressure: \_\_\_\_\_ kPa



Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

**Measurement no. 2:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_

Remarks:

Date:

Time:

Temperature:

°C

Relative humidity:

%

Barometric pressure:

kPa

Remarks:

**Measurement no. 3:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_

Date:   
 Time:   
 Temperature:  °C  
 Relative humidity:  %  
 Barometric pressure:  kPa

**Measurement no. 4:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_

Remarks:

Date:   
 Time:   
 Temperature:  °C  
 Relative humidity:  %  
 Barometric pressure:  kPa

**Measurement no. 5:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	


Evaluator: \_\_\_\_\_

Remarks:

Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

**Measurement no. 6:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_

Remarks:

**Measurement no. 7:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Date:		
Time:		
Temperature:		°C
Relative humidity:		%
Barometric pressure:		kPa

Date:		
Time:		
Temperature:		°C
Relative humidity:		%
Barometric pressure:		kPa

Evaluator: \_\_\_\_\_

Remarks:

Date:		
Time:		
Temperature:		°C
Relative humidity:		%
Barometric pressure:		kPa

Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

**Measurement no. 8:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Average indication ( )
	Indication ( )	Time	Indication ( )	Time	Indication ( )	Time	
						span	

Evaluator: \_\_\_\_\_

Remarks:

Date:		
Time:		
Temperature:		°C
Relative humidity:		%
Barometric pressure:		kPa

**Form 6.19.2 (5 runs) Span stability measurement data for class B**

R60 parts 1&2 Ref.: 8.10.7.11, 5.7.2.6

R60 part 3: 2.2.9

Application no.: \_\_\_\_\_

Load cell model: \_\_\_\_\_

Serial no.: \_\_\_\_\_

$E_{\max}$ : \_\_\_\_\_

$n_{LC}$ : \_\_\_\_\_

$V_{\min}$ : \_\_\_\_\_

Force-generating system: \_\_\_\_\_

Indicating instrument: \_\_\_\_\_

$p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_

Conversion factor, f: \_\_\_\_\_

Minimum test load,  $D_{\min}$ : \_\_\_\_\_

Maximum test load,  $D_{\max}$ : \_\_\_\_\_

- Notes:*
- 1 Span is the result of subtracting the average indication at minimum test load from the average indication at maximum test load.
  - 2 Absolute (not relative) time shall be recorded.

**Table 6.19.2 (5 runs)**

**Measurement no. 1:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Date:

Time:

Temperature:

 °C

Relative humidity:

 %

Barometric pressure:

 kPa

Evaluator: \_\_\_\_\_

Remarks:

**Measurement no. 2:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Date:

Time:

Temperature:

 °C

Relative humidity:

 %

Barometric pressure:

 kPa

Evaluator: \_\_\_\_\_

Remarks:

Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

**Measurement no. 3:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Evaluator: \_\_\_\_\_

Remarks:

Date:

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

**Measurement no. 4:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Evaluator: \_\_\_\_\_

Remarks:

Date:

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

**Measurement no. 5:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

Date:

Evaluator: \_\_\_\_\_

Remarks:

**Measurement no. 6:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Date:

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

Evaluator: \_\_\_\_\_

Remarks:



Report number \_\_\_\_\_

Report page \_\_\_\_ of \_\_\_\_

Report date: \_\_\_\_\_

**Measurement no. 7:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Evaluator: \_\_\_\_\_

Remarks:

Date:

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

**Measurement no. 8:**

Test load (g, kg, or t)	Run no. 1		Run no. 2		Run no. 3		Run no. 4		Run no. 5		Average indication ( )
	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	indication ( )	Time	
										Span	

Evaluator: \_\_\_\_\_

Remarks:

Date:

Time:

Temperature:  °C

Relative humidity:  %

Barometric pressure:  kPa

**Form 6.19.3 Span stability – summary of test results**

R60 parts 1&amp;2 Ref.: 8.10.7.11, 5.7.2.6

R60 part 3: 2.2.9

Application no.: \_\_\_\_\_  
 Load cell model: \_\_\_\_\_  
 Serial no.: \_\_\_\_\_  
 $E_{\max}$ : \_\_\_\_\_  
 $n_{LC}$ : \_\_\_\_\_  
 $v_{\min}$ : \_\_\_\_\_  
 $p_{LC}$ : \_\_\_\_\_ DR: \_\_\_\_\_  
 Force-generating system: \_\_\_\_\_  
 Indicating instrument: \_\_\_\_\_  
 Evaluator: \_\_\_\_\_

**Table 6.19.3**

Measurement no. (see Note 3)	Span		Variation ( $v_{\min}$ )	Maximum allowable variation ( $v_{\min}$ )
	( )	( $v_{\min}$ )		
1				
2				
3				
4				
5				
6				
7				
8				

PASS: ☐ FAIL: ☐

Remarks: